

2015

Refractive Index Sensor Based on a Silica Microsphere Whispering Gallery Mode Resonator

Arun Mallik
Technological University Dublin

Qiang wu
Technological University Dublin, qiang.wu@tudublin.ie

Gerald Farrell
Technological University Dublin, gerald.farrell@tudublin.ie

See next page for additional authors

Follow this and additional works at: <https://arrow.tudublin.ie/engschmanconn>



Part of the [Electrical and Computer Engineering Commons](#), and the [Manufacturing Commons](#)

Recommended Citation

Mallik, A. K, et al. (2015) Refractive Index Sensor Based on a Silica Microsphere Whispering Gallery Mode Resonator. *Recent Advances in Photonics (WRAP), 2015 Workshop on. IEEE, 2015*.doi:10.21427/e0wx-t805

This Conference Paper is brought to you for free and open access by the School of Manufacturing and Design Engineering at ARROW@TU Dublin. It has been accepted for inclusion in Conference Papers by an authorized administrator of ARROW@TU Dublin. For more information, please contact arrow.admin@tudublin.ie, aisling.coyne@tudublin.ie, gerard.connolly@tudublin.ie, vera.kilshaw@tudublin.ie.

Authors

Arun Mallik, Qiang wu, Gerald Farrell, and Yuliya Semenova

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/287330289>

Refractive Index Sensor Based on a Silica Microsphere Whispering Gallery Mode Resonator

Conference Paper · December 2015

DOI: 10.1109/WRAP.2015.7805968

CITATIONS

0

READS

176

4 authors, including:



Arun Mallik

Dublin Institute of Technology

27 PUBLICATIONS 32 CITATIONS

[SEE PROFILE](#)



Qiang Wu

Northumbria University

211 PUBLICATIONS 1,312 CITATIONS

[SEE PROFILE](#)



Yuliya Semenova

Dublin Institute of Technology

256 PUBLICATIONS 1,931 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



Whispering Gallery Mode Fiber Resonators [View project](#)



WGM micro resonator [View project](#)

All content following this page was uploaded by [Arun Mallik](#) on 19 December 2015.

The user has requested enhancement of the downloaded file. All in-text references [underlined in blue](#) are added to the original document and are linked to publications on ResearchGate, letting you access and read them immediately.

Refractive Index Sensor Based on a Silica Microsphere Whispering Gallery Mode Resonator

Arun Kumar Mallik, Qiang Wu, Gerald Farrell, Yuliya Semenova

Photonics Research Center
Dublin Institute of Technology
Dublin 8, Ireland
d13125763@mydit.ie

Abstract— We investigated the excitation of whispering gallery modes (WGMs) in a silica microsphere by evanescent field coupling method using a ~2 micrometer diameter fiber taper. Based on this configuration we have developed a sensitive refractometric sensor and observed a red-shift of the WGM resonances with the increase of the surrounding medium refractive index. A sensitivity of ~114 nanometer per RIU has been achieved in the range of refractive indices from 1.3963 to 1.4004

Keywords— Whispering Gallery Mode, Optical resonator, Optical fiber sensors, Refractive index

I. INTRODUCTION

Evanescent field based optical sensor is one of the most commonly used types of transducers for sensing applications in the fields of liquid, food and water-quality control, health, safety, and environmental monitoring. Among the evanescent field based sensors, whispering gallery mode (WGM) resonators have gained a substantial popularity in recent years due to their high quality factors (Q), low absorption loss and easy and inexpensive fabrication methods. WGMs are high angular momentum modes which can be excited by trapping light propagating inside a dielectric structure with circular symmetry, such as a microsphere, by repeated total internal reflection. When light is reflected at the surface of the resonator, it induces the evanescent wave in the surrounding medium that propagates along the tangent to the surface and extends ~ 200 nm outward [1]. The spectral responses of resonances are strongly dependent on the geometry of the dielectric resonator (diameter, sphericity), optical properties of the resonator material and also on the refractive index (RI) of surrounding the resonator medium, which makes this device suitable for sensing of the surrounding RI [2,3]. WGMs in a silica sphere can be easily excited by trapping a portion of evanescent field propagating through a fiber taper and the changes in the surrounding RI can be measured by monitoring either reflected or transmitted light through the taper [4].

In this paper we demonstrate application of WGMs in a silica microsphere for refractometric sensing. The WGMs are excited in the microsphere by evanescent light coupling using a ~2 μm tapered fiber. Without disturbing the microsphere-taper alignment, a few drops of higher refractive index liquid were added. Resonance wavelength shift was recorded using photo detector with the help of labview programme and a sensitivity of 114 nm/RIU was observed when the RI of the liquid changed from 1.3963 to 1.4004 in real time.

II. THEORY

Electromagnetic field distribution in a dielectric sphere depends on the sphere's effective radius, dielectric loss factor for different modes and the transmission coefficient between the coupled tapered fiber and the sphere. High resolution spectroscopy of whispering gallery modes in a large dielectric sphere ($R \gg \lambda$) was reported by Stephan Schiller et al [5]. For large spheres the resonance frequency of WGM can be expressed as

$$n_s x_l^i = v + \frac{\alpha_i}{2^{1/3}} v^{1/3} - \frac{mp}{\sqrt{m^2-1}} + \frac{3\alpha_i}{10 \times 2^{2/3}} v^{-1/3} + \frac{m^3 p \left(\frac{2p^2-1}{3} \right) \alpha_i}{\frac{1}{2^3} (m^2-1)^{3/2}} v^{-2/3} + 0(v^{-1}) \quad (1)$$

where l , is the angular mode number of the sphere, $v = l + \frac{1}{2}$, $m = n_s/n_e$ is the relative RI between the sphere and the medium in which it is immersed, $p = 1$ for TE modes, $p = 1/m^2$ for TM modes, α_i is the i th zero of Airy function and $x = 2\pi R/\lambda$. The above equation states that RI change of immersion liquid results in a larger spectral shift for a lower angular mode. At the same time broadening in the line width of the mode also takes place. The resonance condition of the sphere is $N\lambda/n_s = 2\pi R$, where N is the integer number of the orbital wavelength. Based on this resonance condition the sensitivity of the resonance wavelength to changes in the

radius ΔR or refractive index Δn_s is given by the following equation [6]:

$$\frac{\Delta\lambda}{\lambda} = \frac{\Delta R}{R} + \frac{\Delta n_s}{n_s} \quad (2)$$

It can be seen that an increase in the radius or the RI both lead to a red shift in the WGM resonance wavelength.

III. EXPERIMENTAL SETUP

The microsphere for our experiments was fabricated at the tip of a standard single mode fiber (Figure 1(a)). The cleaved end of the fiber was put inside a fusion splicer (Sumitomo Type-36). A series of electric arc discharges was applied to the cleaved part of the fiber, so that the tip of the fiber was gradually melted and became spherical in shape due to surface tension (Figure 1(b)). As reported previously in [7] the diameter of the sphere increases with the number of arcs reaching a saturation value around 350 μm . In this experiment spheres with a diameter circa 300 μm were used. The sensitivity ($S=\delta\lambda/\delta n$) of the resonator to the surrounding RI increases with the decrease of the sphere diameter, however as was demonstrated in [3] the decrease in diameter also results in the reduction of the Q- factor. As Q factor implies how many round trips a photon can be travelled inside the sphere before being lost by absorption and scattering. In our experiments we used microsphere with diameters between 220 μm and 320 μm . The main advantage of such a size is ease of fabrication and handling during the experiment. Tapered fiber was fabricated using a customized micro heater brushing technique. A few centimeters of coating length was removed from the fiber before tapering. Then the fiber was placed horizontally using two computer controlled XYZ translational stages pulling the fiber through the micro heater opening. During tapering, translation stages were moved horizontally at the same time fiber was being stretched by the stages. A micrograph of the resulting taper is shown in Figure 1(c). After fabrication two ends of the taper were fixed with UV curable epoxy on the glass slide.

Optical characterization set up is shown in Fig (2). One end of the tapered fiber was connected to the Tunics-plus outside cavity tunable laser. This laser has a capability of wavelength tuning with a resolution of 1 pico meter within the range 1.3963 to 1.4054. A LabView programme was developed to control the tuning of the laser wavelength. The laser output was passed through a motorized polarization controller. The microsphere and tapered fiber were mounted on a xyz nano-metric translation stage. Microsphere was slowly and carefully brought in contact with the tapered fiber for excitation of WGM resonances. The other end of tapered fiber was connected to a high speed InGaAs photo detector (Thorlabs PDA 10CS). The coupling between microsphere and tapered fiber was monitored by a high resolution digital camera.

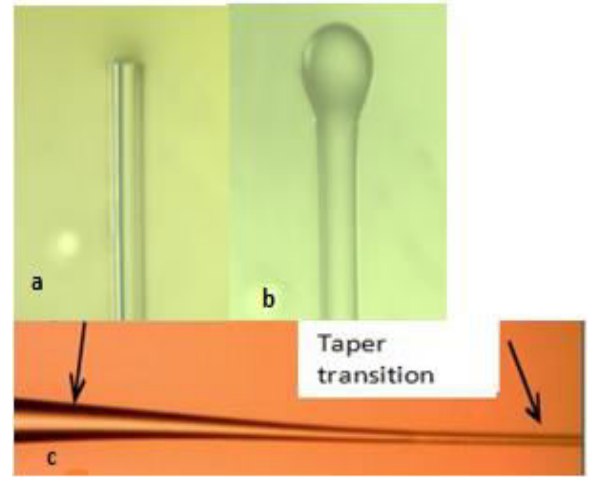


Fig .1. Optical fiber tip before (a) and after (b) applying an electric arc, (c) tapered fiber

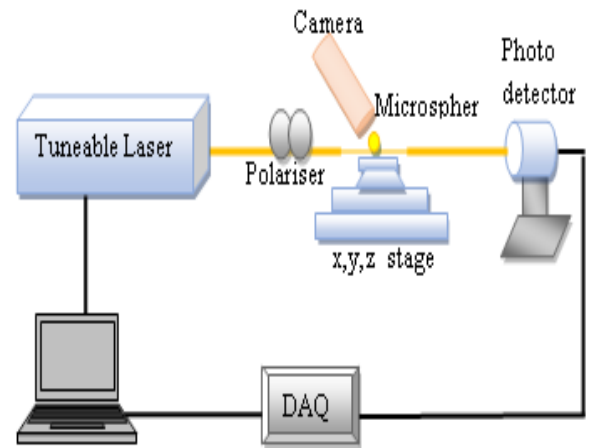


Fig. 2. Experimental setup for microsphere and fiber taper coupling

IV. RESULTS AND DISCUSSION

Before conducting the refractive index sensing experiment, excitation of the WGM resonance was ensured passing the TE polarized laser light through the fiber taper which was evanescently coupled to the equatorial part of the microsphere. The Q factor of the WGM resonance was estimated by measuring the line width of the WGM resonance around 1550 nm as shown in Figure 3. The fundamental WGM corresponds to the dips with the highest extinction ratio. The quality factor can be calculated as $Q = \frac{\lambda_{res}}{\Delta\lambda_{FWHM}}$, where λ_{res} is the wavelength of a resonance, and $\Delta\lambda_{FWHM}$ is the width of the resonant lobe at full-width of half maximum (FWHM). The FWHM is calculated by fitting one of the best resonance dips to a Lorentz equation as shown in the inset of Figure 3. We estimated the FWHM as 0.085 pm at the wavelength of 1550.5345 nm. The corresponding value of the Q- factor is calculated approximately as 1.8×10^7 .

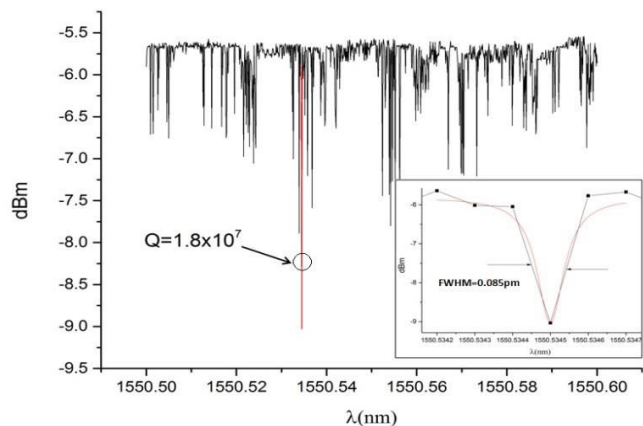


Fig 3: Experimental transmission spectrum for a 270 μm diameter sphere coupled to a $\sim 2\mu\text{m}$ tapered fiber.

For the RI sensing experiment the liquid with refractive index 1.3963 was prepared by mixing of dimethyl sulphoxide with refractive index of 1.4790 and deionized water using a magnetic stirrer. Refractive index of the mixture was measured as 1.3963 by Abbey's refractometer. Few drops of the liquid mixture were carefully placed on the glass slide with the fiber taper. The glass slide was slowly moved upward toward the sphere until the sphere was immersed completely in the liquid without disturbing the coupling between sphere and tapered fiber. The transmission spectrum of immersed

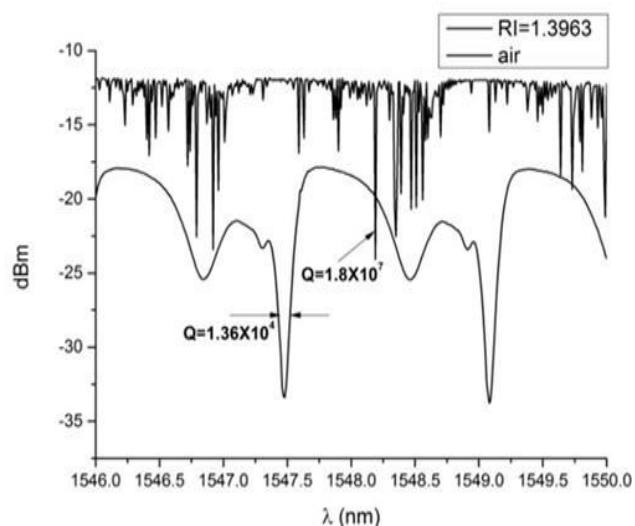


Fig: 4 Real time spectrum of the taper coupled to the microsphere immersed in a liquid of with refractive of 1.3963

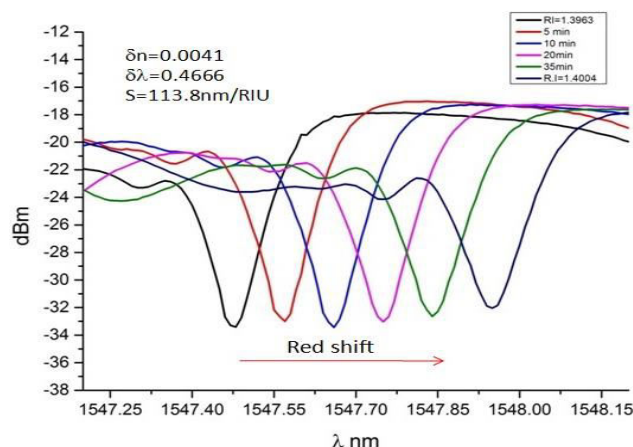


Fig 5: Red shift of 466 pm of WGM spectrum when the refractive index of liquid increases 4×10^{-3}

sphere is shown in Figure 4. It can be clearly noticed from the figure that all other modes vanish after immersing the microsphere in the liquid due to the decrease in refractive index contrast in comparison with the case in air. The Q factor of the immersed in the liquid microsphere is significantly lower (1.36×10^4) compared to that in air (1.8×10^7) and is shown in Fig. 4. Tuning of the surrounding the microsphere refractive index was done by adding few drops of a higher refractive index liquid into the mixture. Simultaneously the WGM spectra were recorded after 5, 10, 20 and 35 min respectively. After 35 min we stopped recording the spectra as there was no further changes in the positions of the WGM resonances. An overall red shift of the WGM resonances 0.466 nm was observed when the refractive index of the liquid was changed from 1.3963 to 1.4004.

V. CONCLUSION

In conclusion, we have reported the observation of refractive index sensing based on a spherical WGM resonator fabricated at the end tip of silica fiber. Maximum demonstrated sensitivity of the WGM sensor to the surrounding refractive index change was 114 nm/RIU in the range of RIs from 1.3963 to 1.4004. This value could be significantly improved by fine tuning the parameters of the microsphere and thus such a sensor could be developed into a microprobe for label-free sensing for various applications.

Acknowledgment

Arun Kumar Mallik would like to acknowledge the support of Dublin Institute of Technology and Fiosraigh Dean of Graduate Students scholarship.

References

- [1] F. Volmer and S. Arnold, "Whispering gallery mode biosensing: label free detection down to single molecules", *Nature methods*, vol. 5, pp. 591-596, June 2008.

- [2] [T. Ioppolo, N. Das, and M. V. Otugen, "Whispering gallery modes of microspheres in the presence of a changing surrounding medium: A new ray-tracing analysis and sensor experiment," J. Appl. Phys., Vol. 107, pp. 103105\(1\)-103105\(8\), Aug. 2010.](#)
- [3] [J. C. Knight, G. Cheung, E Jacques, and T. A. Birks, "Phased-matched excitation of whispering-gallery mode resonances by a fiber taper," Opt. Lett. vol 25 p 1129-1131, 1997.](#)
- [4] [N.M.Hanumegowda, C.J.Stica, B.C.Patel, I.White, and X.Fan, "Refractometric sensors based on microsphere resonators", Appl.Phys.Lett. 87 ,pp.201107-1-201107-3, Nov 2005.](#)
- [5] [S. Schiller, R.L. Byer, "High-resolution spectroscopy of whispering gallery modes in large dielectric spheres", Opt. Lett., vol.15, pp.1138-1140 ,Aug 1991.](#)
- [6] [F. Vollmer, D. Braun, and D. Keng, "Single virus detection from the refractive shift of a whispering gallery mode" Proc. Natl. Acad. Sci. U.S.A, vol.105, pp.20701-20704, Nov 2008.](#)
- [7] [S. Pang, R.E. Beckham, K. E. Meissner, "Quantum dot-embedded microspheres for remote refractive index sensing" , Appl.Phys.Lett.,vol.92,pp.221108, 2008.](#)